





APÉNDICE C

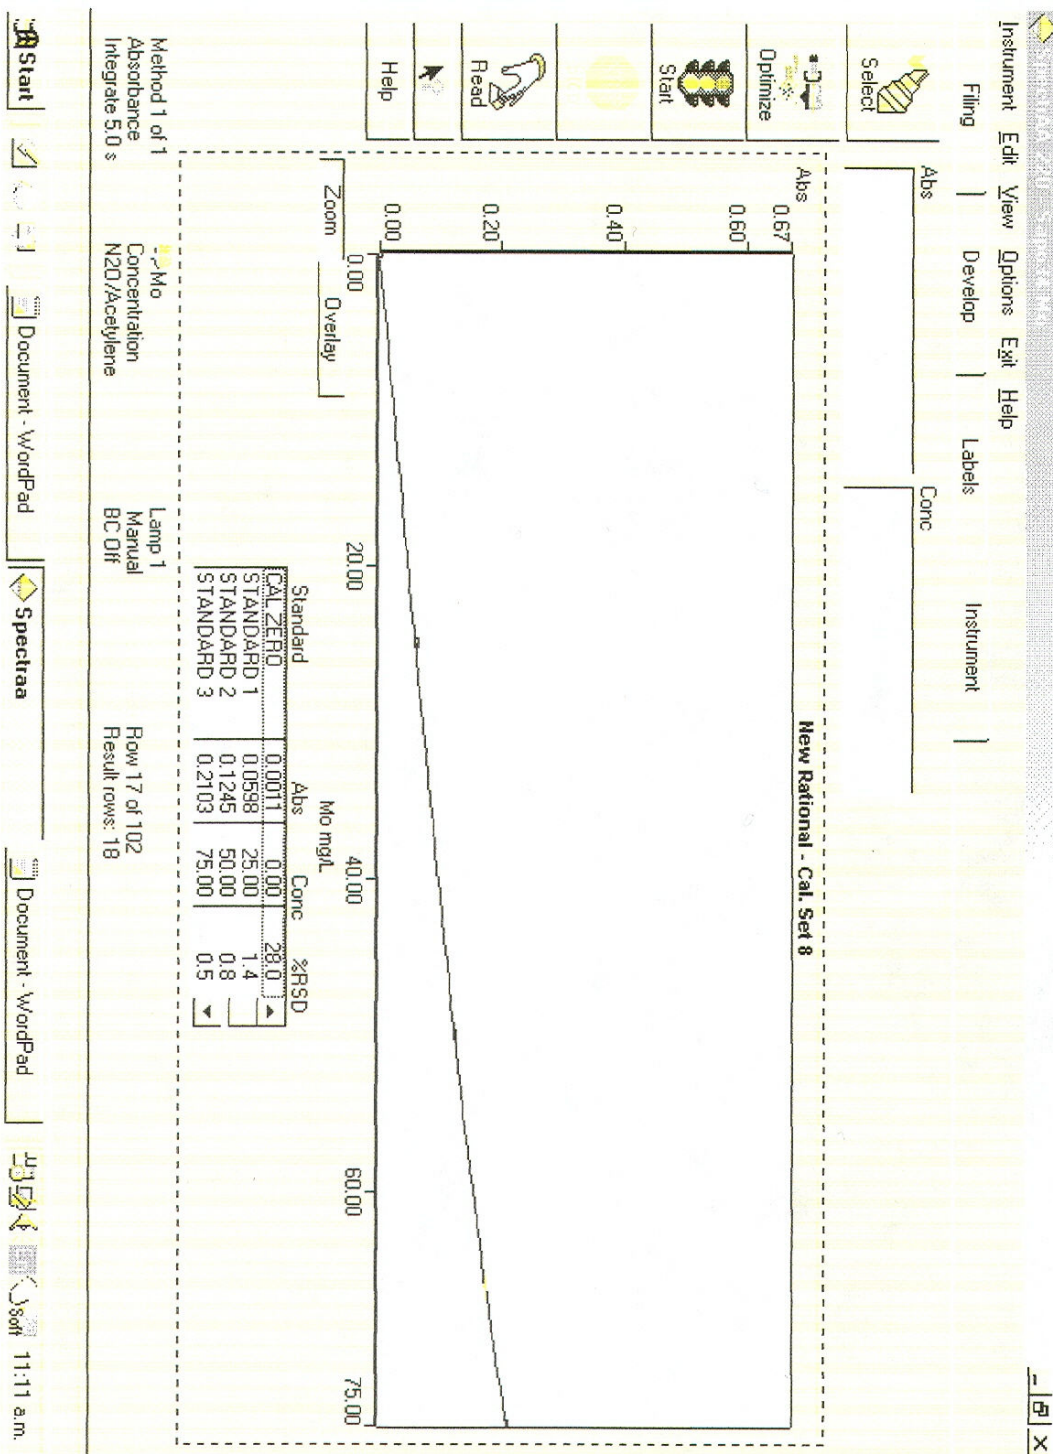

Filing | Develop | Labels | Instrument

Abs Conc

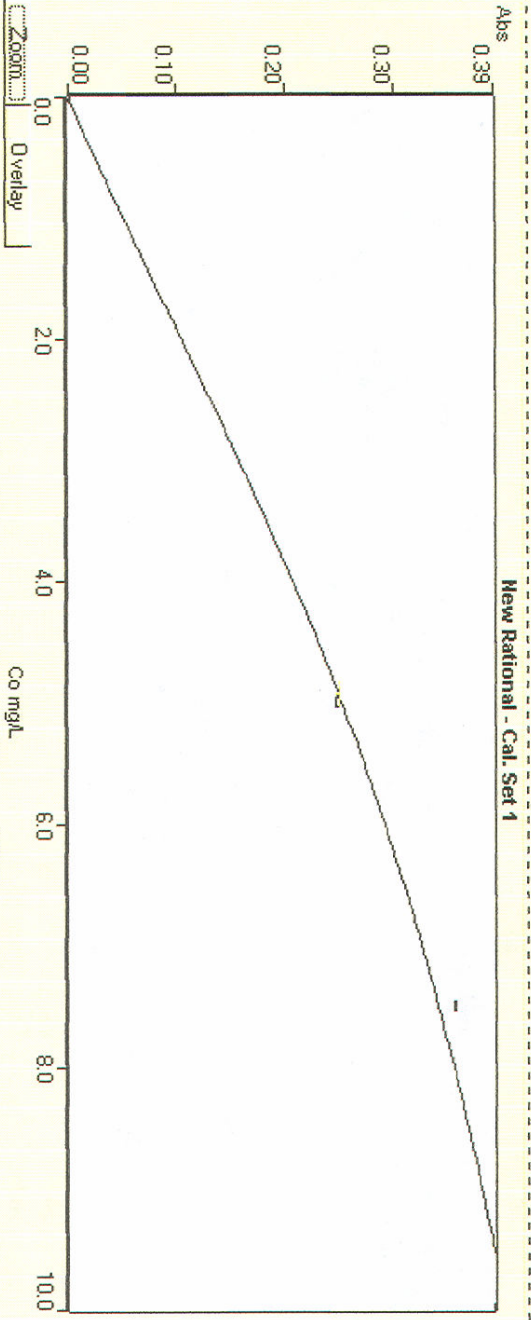

Standard	Abs	Conc	%RSD
CAL ZERO	-0.0009	0.000	11.6
STANDARD 2	0.3635	7.500	0.0
STANDARD 3	0.3911	10.000	0.0

Method 1 of 1
Absorbance
Integrate 5.0 s

Co
Concentration
Air/Acetylene

Lamp 2
Manual
BC Off

Row 4 of 100
Result rows: 6

Worksheet Saved

Start Spectra Document - Wor... 3 1/2 Floppy (A:) Document - Wor... Document - Wor... 10:59 a.m.





Abs Concentración



Optimizar



Empezar




Parar



Leer



Ayuda

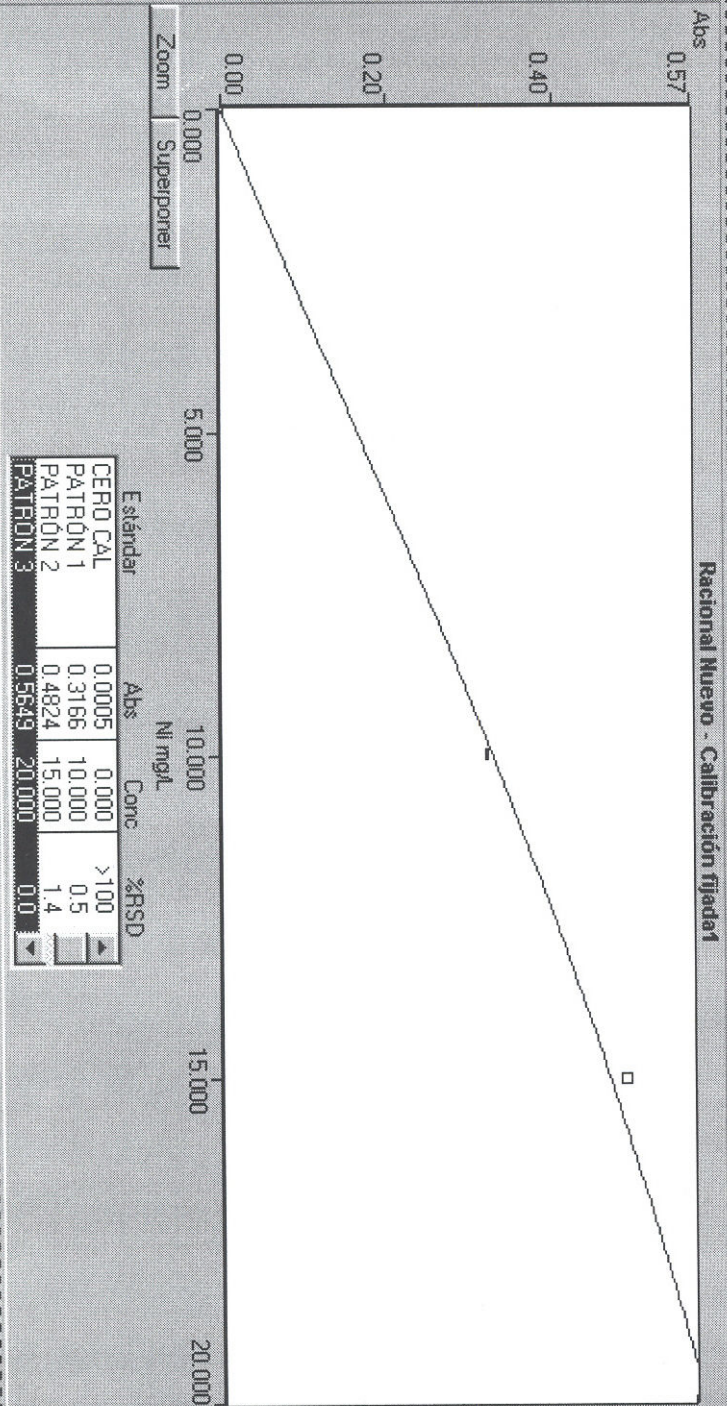

Estándar	Abs	Conc	%RSD
CERO CAL	0.0005	0.000	>100
PATRÓN 1	0.3166	10.000	0.5
PATRÓN 2	0.4824	15.000	1.4
PATRÓN 3	0.5649	20.000	0.0

Método1 de 1
Absorbancia
Integración 5.0 s

Concentración
Ni
Aire/Acuelero

Lámpara 1
Manual
C. Fondo desactivado

Fila 2 de 50
Filas resultado: 3

